

DF 110

Detector of refrigerant gases and hydrogen (H₂)



KEY POINTS

- Detection of all the HCFC and HFC refrigerants
- Detection of mixtures 5% hydrogen - 95% nitrogen (Nidron 5...)
- Heated diode sensor
- 3 modes of sensitivity (high, low and normal)
- Manual and automatic autozero

TECHNICAL FEATURES

Detected gases	HFC: R134a, R404a, R407c, R410a, R32, R422a/b/c/d, R425a, R507a, R125 HCFC: R22 CFC: R12, R502 Others: H ₂ , R290, R600a, HFO-1234yf, HFO-1234ze
Measuring element	Semi-conductor sensor
Display	13 leds: - 8 for the graphic visualization of thresholds - 3 for the sensitivity of detection - 2 for the battery level and manual autozero
Indication	LED: gradual lighting up when the gas concentration increases Audible : the beep frequency increases when the gas concentration increases
Probe	Flexible, 300 mm length
Autonomy	> 12 hours
Housing	Anti-choc ABS, protection IP54
Keypad	3 keys
European directives	2014/30/EU EMC ; 2014/35/EU Low Voltage ; 2011/65/EU RoHS II ; 2012/19/EU WEEE
Power supply	4 AAA LR03 1.5 V batteries
Ambiance	Neutral gas
Conditions of use (°C, %RH, m)	From 0 to +50 °C. In non condensing conditions. From 0 to 2000 m.
Storage temperature	From -20 to +80 °C
Auto-extinction	15 min
Weight	295 g

SPECIFICATIONS

Mode	Indicative measuring range (g/an)	Visual alarm
Low sensitivity ("B" on the device)	From 0 to 300 g/an	All the leds (8) for 300 g/an
Normal sensitivity ("Norm" on the device)	From 0 to 30 g/an	All the leds (8) for 30 g/an
High sensitivity ("H" on the device)	From 0 to 3 g/an	All the leds (8) for 3 g/an




REGLEMENTATIONS

The refrigerant gas detector complied with the EN 14624 standard that determines the following points:

- **Minimum threshold of sensitivity:**
Fixed : < 1 g / year at 3 mm
In moving air : 2 g / year, 2 cm / s at 3 mm
- **Minimum time of detection (1 g / year):** 1 second
- **Autozero:** 2 seconds
- **Recuperation time after exposition:** from 1 to 10 seconds (depending on detection level and threshold of sensitivity)

SIZE

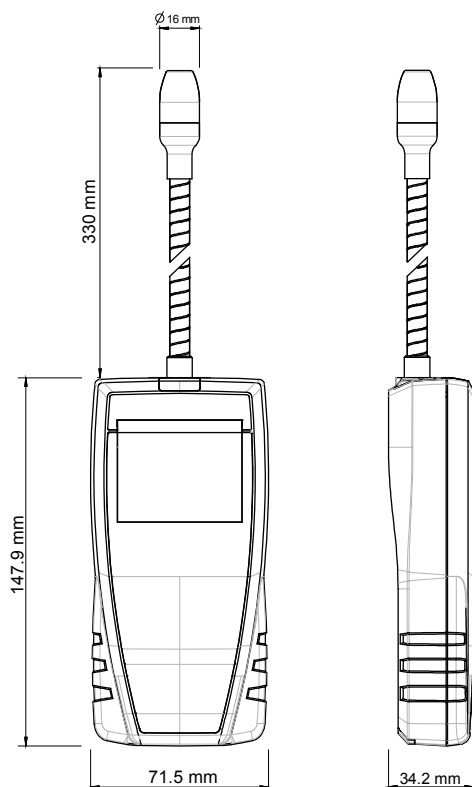

MAINTENANCE

We realise the check, adjustment and maintenance of your devices to guarantee a constant quality level of your measurements. According to the quality assurances standards, we recommend a yearly checking. We recommend to check regularly that the nozzle of the detector and its filter are clean in order to guarantee the performances of the device.

WARRANTY

Instruments have 1-year guarantee for any manufacturing defect (return to our After-Sales Service required for appraisal).

SUPPLIED WITH

Devices are supplied with:

- Verification certificate
- Transport case
- Test sample containing refrigerant gas
- Filter



ACCESSORIES

CQD: Magnetic protective housing



MT 51: ABS transport case



大華高科股份有限公司

www.taiwah.com.tw info@taiwah.com.tw

台北 TEL: (02) 2592 - 5119 Fax: (02) 2592- 3577

台中 TEL: (04) 2707 - 2269 Fax: (04) 2707- 1799

台南 TEL: (06) 243 - 2338 Fax: (06) 243 - 2339

KIMO® 為 KIMO 儀器公司的註冊商標。

資料中任何商標和圖片為本公司版權所有。未經本公司書面許可不得以任何形式複製，轉印，發行或儲存資料中所包含的訊息。本資料如有變更，恕不另行通知。