

Thermo-hygrometer HD 110



KEY POINTS

- Easy to use
- Adjustable backlight
- Hold-min-max functions
- Selection of units

TECHNICAL FEATURES

Measuring element	Digital sensor (CMOS)
Display	4 lines, LCD technology. Sizes 50 x 36 mm 2 lines of 5 digits with 7 segments (value) 2 lines of 5 digits with 16 segments (units)
Cable	Coiled, length 0.45 m, expanding to 2.4 m
Housing	ABS, IP54 protection
Keypad	5 keys
European directives	2014/30/EU EMC; 2014/35/EU Low Voltage; 2011/65/EU RoHS II; 2012/19/EU WEEE
Power supply	4 batteries AAA LR03 1.5 V
Battery life	150 hours
Ambiance	Neutral gas
Conditions of use (instrument) (°C, %RH, m)	From -10 to +50°C. In non condensing conditions. From 0 to 2000 m.
Operating temperature (probe)	From -20 to +70°C
Storage temperature	From -20 to +80°C
Auto shut-off	Adjustable from 0 to 120 min
Weight	310 g



SPECIFICATIONS

Measuring units	Measuring range	Accuracy ¹	Resolution
Relative humidity			
%HR	From 0 to 100%HR	Accuracy* (Repeatability, linearity, hysteresys) : ±1.8%HR (from 15°C to 25°C) Factory calibration uncertainty : ±0.88%HR Drift linked to the temperature : ±0.04 x (T-20) %HR (if T < 15°C or T > 25°C)	0.1%HR
Dew point			
°C _{td} , °F _{td}	From -40 to +70°C _{td}	±0.8% of reading ±0.6°C _{td}	0.1°C _{td}
Ambient temperature			
°C, °F	From -20 to +70°C	±0.4% of reading ±0.3°C	0.1°C


¹All accuracies indicated in this document were stated in laboratory conditions and can be guaranteed for measurements carried out in the same conditions, or carried out with required compensation. As per NFX 15-113 and the Charter 2000/2001 HYGROMETERS, GAL (Guaranteed Accuracy Limit) which has been calculated with a coverage factor value of 2 is ±2.68%RH between 15 and 25°C on the measuring range from 5 to 95%RH. Sensor drift is less than 1%RH/year.

*Except class 110 S

FUNCTIONS

- Relative humidity, dew point and temperature measurements
- Selection of units (temperature and dew point)
- Hold Function
- Display of minimum and maximum values
- Configurable auto shut-off
- Backlight


DIMENSIONS

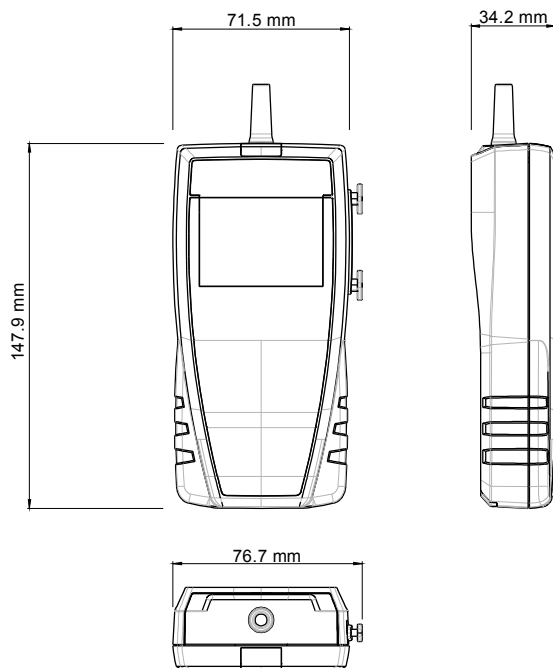

OPERATING PRINCIPLES

Measurement of capacitive hygrometry

On the capacitive probes, a sensitive polymer layer reacts with the humidity present between two metal layers which cover a glass substract. Water absorption is a function of relative humidity of the surrounding environment, and modifies the dielectric constant. The measured signal is directly proportional to the relative humidity and independent on the ambient pressure.

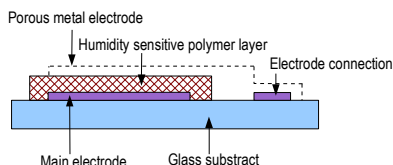

$$C(RH) = \frac{\xi_{RH} \times \xi_0 \times A}{d}$$

C	Capacity of relative humidity sensor	A	Electrodes area
ξ_{RH}	Relative dielectric permittivity, humidity dependent	d	Electrodes spacing
ξ_0	Void permittivity	HR	Relative humidity

Semiconductor temperature sensor

The direct tension of a silicon diode is dependent on the temperature, in accordance with the following equation :

$$V_{BE} = V_{G0} (1 - T/T_0) + V_{BE0} (T/T_0) + (nKT/q) \ln(T_0/T) + (KT/q) \ln(IC/IC_0)$$

T = Temperature in Kelvin

V_{G0} = Voltage of the band gap at the absolute zero

V_{BE0} = Voltage of the band gap at T_0 and IC_0

K = Boltzmann constant

q = charge of an electron

n = Dependent constant of the instrument

SUPPLIED WITH

- The instruments are supplied with:
- Hygrometry probe Ø13 mm, 110 mm length
 - Calibration certificate*
 - Transport case (ref: ST 110)



* Except class 110 S

ACCESSORIES

CQ 15: Magnetic protective housing



RTE: Telescopic extension
Length 1m, with index at $\pm 90^\circ$

MT 51: ABS transport case



MAINTENANCE

We carry out calibration, adjustment and maintenance of your instruments to guarantee a constant level of quality of your measurements. As part of Quality Assurance Standards, we recommend you to carry out an annual verification.

GUARANTEE

Instruments have 1-year guarantee for any manufacturing defect (return to our After-Sales Service required for appraisal).

大華高科股份有限公司

www.taiwah.com.tw info@taiwah.com.tw

台北 TEL: (02) 2592 - 5119 Fax: (02) 2592- 3577

台中 TEL: (04) 2707 - 2269 Fax: (04) 2707- 1799

台南 TEL: (06) 243 - 2338 Fax: (06) 243 - 2339

KIMO® 為 KIMO 儀器公司的註冊商標。

資料中任何商標和圖片為本公司版權所有。未經本公司書面許可不得以任形式複製，轉印，發行或儲存資料中所包含的訊息。本資料如有變更，恕不另行通知。