

## Vane probe thermo-anemometer LV 110 – LV 111 – LV 117



### KEY POINTS

- Airflow calculation
- Automatic average
- Hold-min-max function
- Selection of units

### TECHNICAL FEATURES

<b>Measuring elements</b>	<b>Air velocity:</b> Hall effect sensor <b>Ambient temperature:</b> NTC sensor
<b>Display</b>	4 lines, LCD technology. Sizes 50 x 36 mm 2 lines of 5 digits with 7 segments (value) 2 lines de 5 digits with 16 segments (unit)
<b>Vane probe diameter</b>	<b>LV111:</b> Ø14 mm / <b>LV117:</b> Ø70 mm / <b>LV110:</b> Ø100 mm
<b>Cable</b>	Coiled, 0.45 m length, extension: 2.4 m
<b>Housing</b>	ABS, IP54 protection
<b>Keypad</b>	5 keys
<b>European directives</b>	2014/30/EU EMC; 2014/35/EU Low Voltage; 2011/65/EU RoHS II; 2012/19/EU WEEE
<b>Power supply</b>	4 batteries AAA LR03 1.5 V
<b>Battery life</b>	58 hours**
<b>Ambience</b>	Neutral gas
<b>Conditions of use (instrument) (°C, %RH, m)</b>	From 0 to +50°C. In non condensing conditions. From 0 to 2000 m.
<b>Operating temperature (probe)</b>	From 0 to +50°C
<b>Storage temperature</b>	From -20 to +80°C
<b>Auto shut-off</b>	Adjustable from 0 to 120 min
<b>Weight</b>	390 g



Ø100 mm vane probe

Ø70 mm vane probe

Ø14 mm vane probe

### SPECIFICATIONS

Models	Measuring units	Measuring range	Accuracy <sup>1</sup>	Resolution
<b>Air velocity</b>				
LV111: Ø14 mm	m/s, fpm, km/h	From 0.8 to 25 m/s	From 0.8 to 3 m/s: ±3% of reading ±0.1 m/s From 3.1 to 25 m/s: ±1% of reading ±0.3 m/s	0.1 m/s
LV110: Ø100 mm	m/s, fpm, km/h	From 0.3 to 35 m/s	From 0.3 to 3 m/s: ±3% of reading ±0.1 m/s From 3.1 to 35 m/s: ±1% of reading ±0.3 m/s	0.01 m/s 0.1 m/s
LV117: Ø70 mm	m/s, fpm, km/h	From 0.4 0 to 35 m/s	From 0.4 to 3 m/s: ±3% of reading ±0.1 m/s From 3.1 to 35 m/s: ±1% of reading ±0.3 m/s	0.1 m/s
<b>Airflow</b>				
All models	m³/h, cfm, l/s, m³/s	From 0 to 99 999 m³/h	±3% of reading ±0.03 * area (cm²)	1 m³/h
<b>Temperature</b>				
All models	°C, °F	From -20 to +80°C	±0.4% of reading ±0.3°C	0.1°C

### FUNCTIONS


- Airflow calculation
- Airflow calculation with cone (LV110/117)
- Automatic average
- Selection of units (air velocity, airflow and temperature)
- Hold function
- Display of minimum and maximum values
- Configurable auto shut-off
- Backlight
- Detection of flow direction (LV110/117)
- Selection of the type of cone
- Dimensions of rectangular and circular duct

\* Except class 110 S

\*\*Battery life given at 20°C with alkaline batteries

<sup>1</sup>All the accuracies indicated in this technical data sheet were stated in laboratory conditions, and can be guaranteed for measurements carried out in the same conditions, or carried out with calibration compensation


## DIMENSIONS

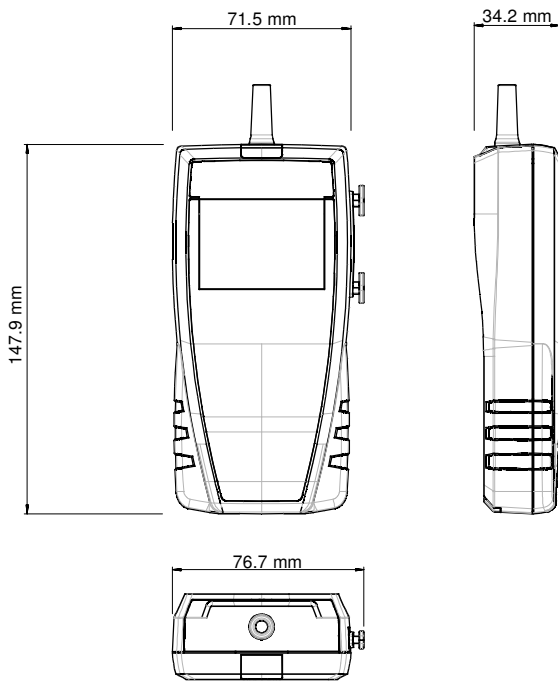

## OPERATING PRINCIPLES

### Air velocity: Hall effect sensor

Rotation of the vane probe leads to a circular magnet of 8 poles. A dual Hall effect sensor, placed next to the magnet captures the signals of magnetic field polarity transition. The sensor signal is converted to electrical frequency and is proportional to the rotation velocity of the vane probe. Signal chronology allows to determine the rotation direction.

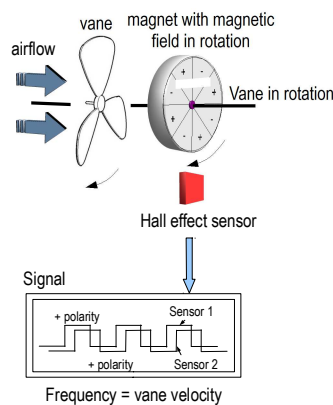

### Thermometer: NTC probe

Negative temperature coefficient probes are thermistors with a resistance that decreases with temperature according to the equation below:

$$R_{(T)} = R_{(T_0)} e^{\left( \frac{\alpha}{100} \times (T_0 + 273.15)^2 \times \left( \frac{1}{T + 273.5} - \frac{1}{T_0 + 273.5} \right) \right)}$$

$R_T$  = resistance sensor value at temperature  $T$

$R_{(T_0)}$  = resistance sensor value at reference temperature  $T_0$

$T$  and  $T_0$  in °C

$\alpha$  and  $T_0$  sensor specific constants

## SUPPLIED WITH

- Instruments are supplied with:
- LV 111: vane probe Ø14 mm
  - LV 117: vane probe Ø70 mm
  - LV 110: vane probe Ø100 mm
  - Calibration certificate\*
  - Transport case (ref.: ST 110)



\* Except class 110 S

## ACCESSORIES

**CQ 15:** Magnetic protective housing



**RTE:** Telescopic extension, length 1m, with index at ±90°

**K 25 – 85:** Airflow cones for anemometer LV 110



**MT 51:** ABS transport case



## MAINTENANCE

We carry out calibration, adjustment and maintenance of your instruments to guarantee a constant level of quality of your measurements. As part of Quality Assurance Standards, we recommend you to carry out a yearly checking.

## WARRANTY

Instruments have 1-year guarantee for any manufacturing defect (return to our After-Sales Service required for appraisal).

# 大華高科股份有限公司

[www.taiwah.com.tw](http://www.taiwah.com.tw) [info@taiwah.com.tw](mailto:info@taiwah.com.tw)

台北 TEL: (02) 2592 - 5119 Fax: (02) 2592 - 3577

台中 TEL: (04) 2707 - 2269 Fax: (04) 2707 - 1799

台南 TEL: (06) 243 - 2338 Fax: (06) 243 - 2339

KIMO® 為 KIMO 儀器公司的註冊商標。

資料中任何商標和圖片為本公司版權所有。未經本公司書面許可不得以任形式複製、轉印、發行或儲存資料中所包含的訊息。本資料如有變更，恕不另行通知。